



IJEAST

INTERNATIONAL JOURNAL
OF ENGINEERING APPLIED SCIENCE
AND TECHNOLOGY



VOLUME : 1 ISSUE : 8 Print / Issue Publication Date: 09-Oct-2016



ISSN : 2455-2143



Indexed In



WWW.IJEAST.COM

editor@ijeast.com



DESIGNING OF MICROSTRIP ANTENNA FOR BIOMEDICAL APPLICATION

Ravindra Parihar
ITM University
Gwalior, India

Anshul Agrawal
ITM University
Gwalior, India

Abstract – Microstrip Patch antennas currently are receiving significant scientific researcher's interest for integration into the implantable medical devices and radio-frequency (RF)-enabled biotelemetry, because of their high flexibility in design, conformability, shape and size. Various techniques have been used so far to design such antennas for different type of diseases. This paper is an output of a detailed survey of various available techniques. The objective of this paper is to propose an antenna which can be used in treating disease like tumors and hyperthermia.

Keywords – IMD, Biomedical telemetry, MPA, Biomedical Applications.

I. INTRODUCTION

Technology modifies each day by a large group of thinkers and researchers of engineering expeditiously. Every aspect of life is greatly affected by it. Human life is getting easier everyday due to new advancements done by the people of science. Especially, when the main interest of a research topic is human life, the topic becomes relatively popular. When engineering is projected on biology and human life, the result becomes medical electronics, which might be one of the popular subjects of research due to its main interest: Human body.

Especially in the area of cancer imaging, scientists work of numerous proposals about the imaging problem and keep discovering new features about solving one of the most deadly diseases in the world.

Hyperthermia is a way to treat cancer tissues with enhancing the temperature of a part of the body within the range 42-45 °C. This technique has been shown to be an effective treatment for some cancers in combination with radiotherapy and chemotherapy. For treatment of tumours which are located close to the surface of the body, the electromagnetic field energy is applied through external antennas (applicators) [1], [2], [3].

Instead of treating any disease, prevention is far better option. Millions of people worldwide depend upon implantable medical devices to support and improve the quality of their lives. RF-linked implantable medical devices are already in use for a wide variety of applications, including temperature monitors [4], pacemakers and cardioverter defibrillators [5],

functional electrical stimulators (FES) [6], blood-glucose sensors [7], and cochlear [8] and retinal [9] implants. As technology continues to evolve, new implantable medical devices are being developed, and their use is expected to rapidly increase from an already large base.


Until recently, no globally accepted frequency band had been dedicated to biotelemetry for implantable medical devices. The situation changed with the ITU-R Recommendation SA.1346 [10], which outlined the use of the 402.0- 405.0 MHz frequency band for Medical Implant Communications Systems (MICS).

However, focus is on the MICS band, because of its advantages of being available worldwide and being feasible with low-power and low-cost circuits, reliably supporting high-data-rate transmissions, falling within a relatively low-noise portion of the spectrum, lending itself to small antenna designs, and acceptably propagating through human tissue.

II. METHODOLOGY

It has been found in previous research that the best frequency range for treating cancer and hyperthermia related critical diseases is 0.4 to 1.5 GHz. whereas the MICS has the range of 0.402 to 0.405GHz and breast cancer has the range of frequency for treatment is 1 to 1.5GHz. So the proposed antenna is designed on 1 GHz frequency.

The front side of the antenna has a feed line with changing width which is connected to the main radiating strip.

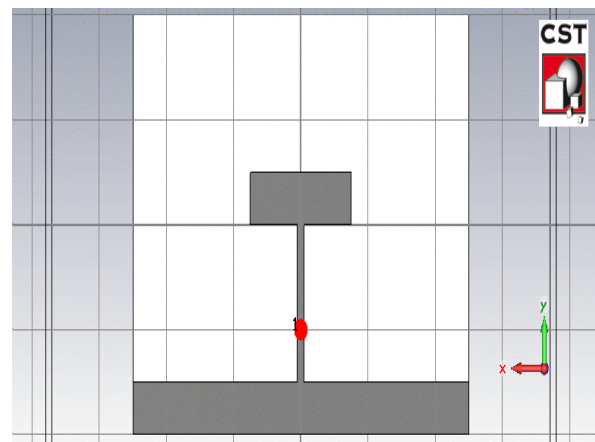

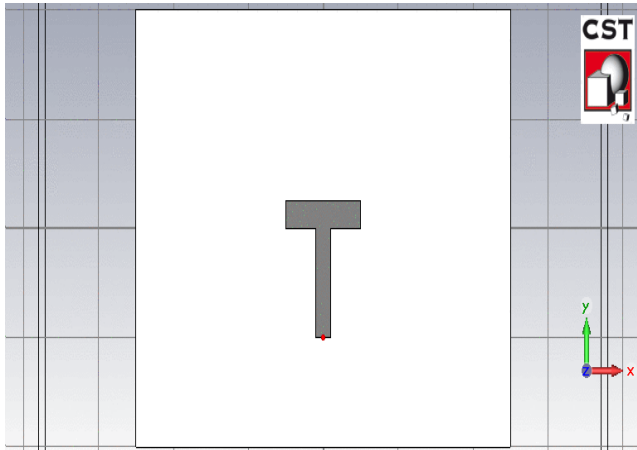


Figure 1. Back and front side of the proposed antenna, inspired by meandered antenna.

This proposed design is inspired by yagi uda antenna proposed by Adela [11], and this proposed antenna will be radiating in as required 1 GHz frequency. The proposed antenna having its PCB structure of 50X50 mm and having a T shaped radiating structure whereas an extended T shaped ground structure. The ground is also can be represented as parallel plates like the one we have in yagi uda antenna, but here in this structure a narrow strip was used to connect these both plates. This strip was used so that a sudden change in width can enhance the radiation from the antenna plane. FR4 lossy was used as a substrate having height 1.6mm and having dielectric constant of 4.3.

Following is the simulated result of the proposed antenna.

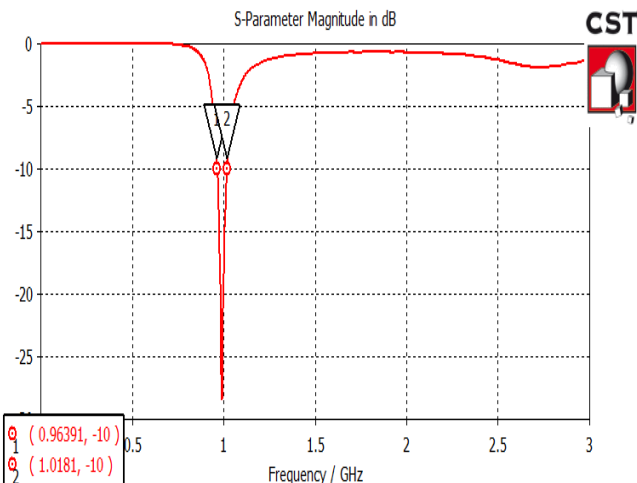


Figure 2. Simulated result of the proposed antenna, showing return loss of -28 dB and bandwidth of 54 MHz

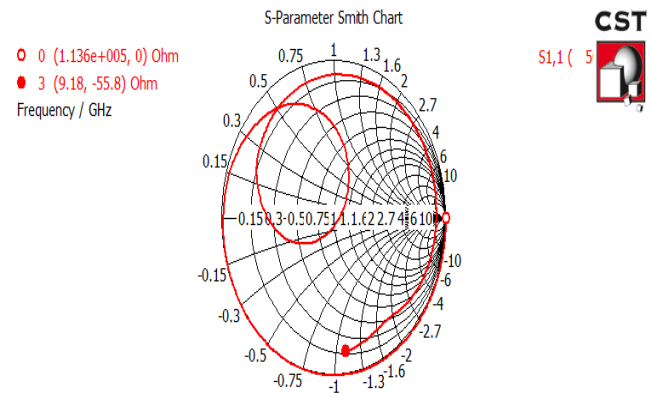


Figure 3. Smith Chart of the simulated patch antenna.

This simulated result shows the return loss of the proposed design showing the return loss of -28dB, which is sufficient enough to treat breast cancer by using imaging technique and can be used in treating hyperthermia as well. Because the range of frequency for such biomedical application is 1 to 1.5GHz.

III. CONCLUSION

A small, single band microstrip antenna is presented. Yagi Uda type of radiator and same type of ground plane are designed. The antenna produced acceptable characteristics when compared to the requirements surveyed from various research papers. This proposed design can also be modified up to a next level, like enhancement of bandwidth, conversion into multi bands and even smaller sizes to reduce the volume of measurement system in general. The proposed antenna has advantages like wide angular width and small size which makes it realizable for the proposed job. The antenna will be crafted and further analyses will be done to understand its capabilities in a realistic case.

IV. REFERENCES

- [1] S. Curto, P. McEvoy, M. J. Ammann, "Compact patch antenna for electromagnetic interaction with human tissue at 434 MHz," IEEE Trans, Antennas Propag. Vol. 57, no. 9, Sep. 2009.
- [2] M. M. Paulides, J. F. Bakker, N. Chavannes, and G. C. Van Rhooen, "A patch antenna design for application in a phased-array and neck hyperthermia applicator," IEEE Trans. Biomed. Eng., vol. 54, no. 11, pp. 2057-2063, Nov. 2007.
- [3] I. J. Bahl, S. S. Stuchly, J. J. W. Lagendijk, M. A. Stuchly, "Microstrip loop radiators for medical applications", IEEE. TRANS. Microw. Theory Tech., vol. 30, no. 7, pp. 1090-1093, Jul. 1982.
- [4] W. G. Scanlon, N. E. Evans, and Z. M. McCreesh, "RF Performance of a 418 MHz Radio Telemetry Packaged for

- Human Vaginal Placement,” IEEE Transactions on Biomedical Engineering, 44, 5, May 1997, pp. 427-430.
- [5] D. Wessels, “Implantable Pacemakers and Defibrillators: Device Overview and EMI Considerations,” Proceedings of the IEEE International Symposium on Electromagnetic Compatibility (EMC 2002), August 2002.
 - [6] K. Guillory and R. A. Normann, “A 100-Channel System for Real Time Detection and Storage of Extracellular Spike Waveforms,” Journal of Neuroscience Methods, 91, 1999 pp. 21-29.
 - [7] M. C. Shults, R. K. Rhodes, S. J. Updike, B. J. Gilligan, and W. N. Reining, “A Telemetry-Instrumentation System for Monitoring Multiple Subcutaneously Implanted Glucose Sensors,” IEEE Transactions on Biomedical Engineering, 41, 10, October 1994, pp. 937-942.
 - [8] T. Buchegger, G. Obberger, A. Reizenhahn, E. Hochmair, A. Stelzer, and A. Springer, “Ultra-Wideband Transceivers for Cochlear Implants,” EURASIP Journal on Applied Signal Processing, 18, 2005, pp. 3069-3075.
 - [9] K. Gosalia, G. Lazzi, and M. Humayun, “Investigation of Microwave Data Telemetry Link for a Retinal Prosthesis,” IEEE Transactions on Microwave Theory and Techniques, 52, 8, August 2004, pp.1925-1932.
 - [10] “International Telecommunications Union-Radio communications (ITU-R), Radio Regulations, SA.1346,” ITU, Geneva, Switzerland; available online: <http://itu.int/home>.
 - [11] Adela, B.B, Mestrom, R.M.C., Paulides, M.M., Smolders, AB. "An MR-compatible Printed Yagi-Uda Antenna for a Phased Array Hyperthermia Applicator" 7th European Conference on Antennas and Propagation (EuCAP). 1142-1/46,2013.

IJEAST

INTERNATIONAL JOURNAL
OF ENGINEERING APPLIED SCIENCE
AND TECHNOLOGY

ABOUT IJEAST

International Journal of Engineering Applied Science and Technology (IJEAST) is a peer-reviewed, open access journal that publishes high-quality research papers in the field of Engineering, Applied Science and Technology.

IJEAST aims to provide a platform for researchers, academicians, and professionals to share their innovative ideas, research findings, and practical experiences with the global scientific community.

FOCUS AREAS

- Engineering
- Applied Science
- Technology
- Innovation & Development
- Interdisciplinary Studies



PEER REVIEWED

All submissions are rigorously peer reviewed to ensure quality.



OPEN ACCESS

Free and unrestricted access to research for all.



GLOBAL REACH

Connecting researchers and professionals worldwide.



TIMELY PUBLICATION

We ensure a swift and efficient publication process.



For more information, visit our website

www.ijeast.com



INTERNATIONAL JOURNAL
OF ENGINEERING APPLIED SCIENCE
AND TECHNOLOGY

✉ editor@ijeast.com

🌐 www.ijeast.com

📍 India



2455-2143